

Dr. Anders Berg, Vice-Chair and Head of CLIA & Lab Operations, Cedars Sinai Medical Center

Don't stand still. Skate to the puck!

Self-collected
Lab Quality Plasma
ANYWHERE



Expand Your Market Access


GATTACO™ BENEFITS	Testing Labs	Clinical Studies	ဗုံ Point-of-Use			
Anywhere Convenience	Remove lab visits	Increase participant diversity & retention	Access users directly			
Lab-Quality Ready to Use	Fewer steps, less sample prep error	Fewer steps, less sample prep error	Provide plasma- ready sample			
Easy to Integrate	Streamline workflow	Streamline workflow	Fits existing tests			
Cost Effective	Less backend logistics	Eliminate phiebotomist	Eliminate phiebotomist			



The A-PON device removes the need for phlebotomy, and easily allows consumers to convert fingerstick blood to liquid plasma in under 3 minutes without any specialized knowledge or equipment.

The plasma obtained fits seamlessly into existing testing workflows without changing established thresholds.

Seamlessy Fits Your Workflow

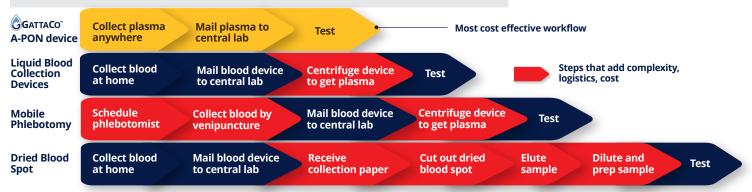


It's easy. Try it now.

gattaco.com

See video, data. Contact us:



Covid-19 Neutralizing Antibody Assay (Natural and Spiked Blood Samples)

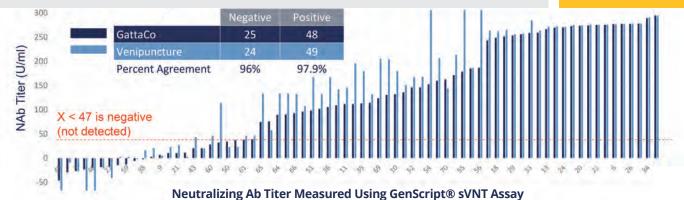

Kidney Disease Panel with Proprietary BioMarkers

STUDY	GLUCOSE		POTASSIUM		CREATININE		CKD-BIOMARKER			GLYCEMIC-BIOMARKER					
	CONTROL	GATTACO	24HR	CONTROL	GATTACO	24HR	CONTROL	GATTACO	24HR	CONTROL	GATTACO	24HR	CONTROL	GATTACO	24HR
1	79.7	77.0	57.3	3.9	4.3	6.9	0.7	0.8	0.7	3.9	4.1	3:8	13.5	13.4	13.4
2	162.7	152.3	144.3	4.0	4.8	6.1	0.9	0.8	0.8	5.4	5.4	5.5	15.5	15.5	15.6
3	83.0	83.0	64.0	3.8	4.5	7.6	0.7	0.7	0.6	4.4	4.1	4.3	12.4	12.4	12.2
4	81.7	80.3	60.0	4.8	5.1	8.1	1.0	0.9	1,0	4.8	0.0	4.9	13.5	13.6	13.7
5	80.0	77.0	56.0	4.0	4.5	7.9	1.1	LI	1.1	4.0	3.6	3.9	14.0	14/1	14.2

Study performed with CLIA Lab partner. All samples are Li-Heparin plasma.

- "Control" is plasma separated by centrifuge immediately after blood collection.
- $\cdot \text{``GattaCo''} \text{ is plasma separated immediately after blood collection using the GattaCo device.}$
- "24hr" is plasma separated infinediately after blood collection using the separated by centrifuge 24 hours after blood collection.

©2022 GattaCo All Rights Reserved. A-PON device is for Research Use Only Not FDA-Cleared